


SURGICAL C-ARM TABLE - 846

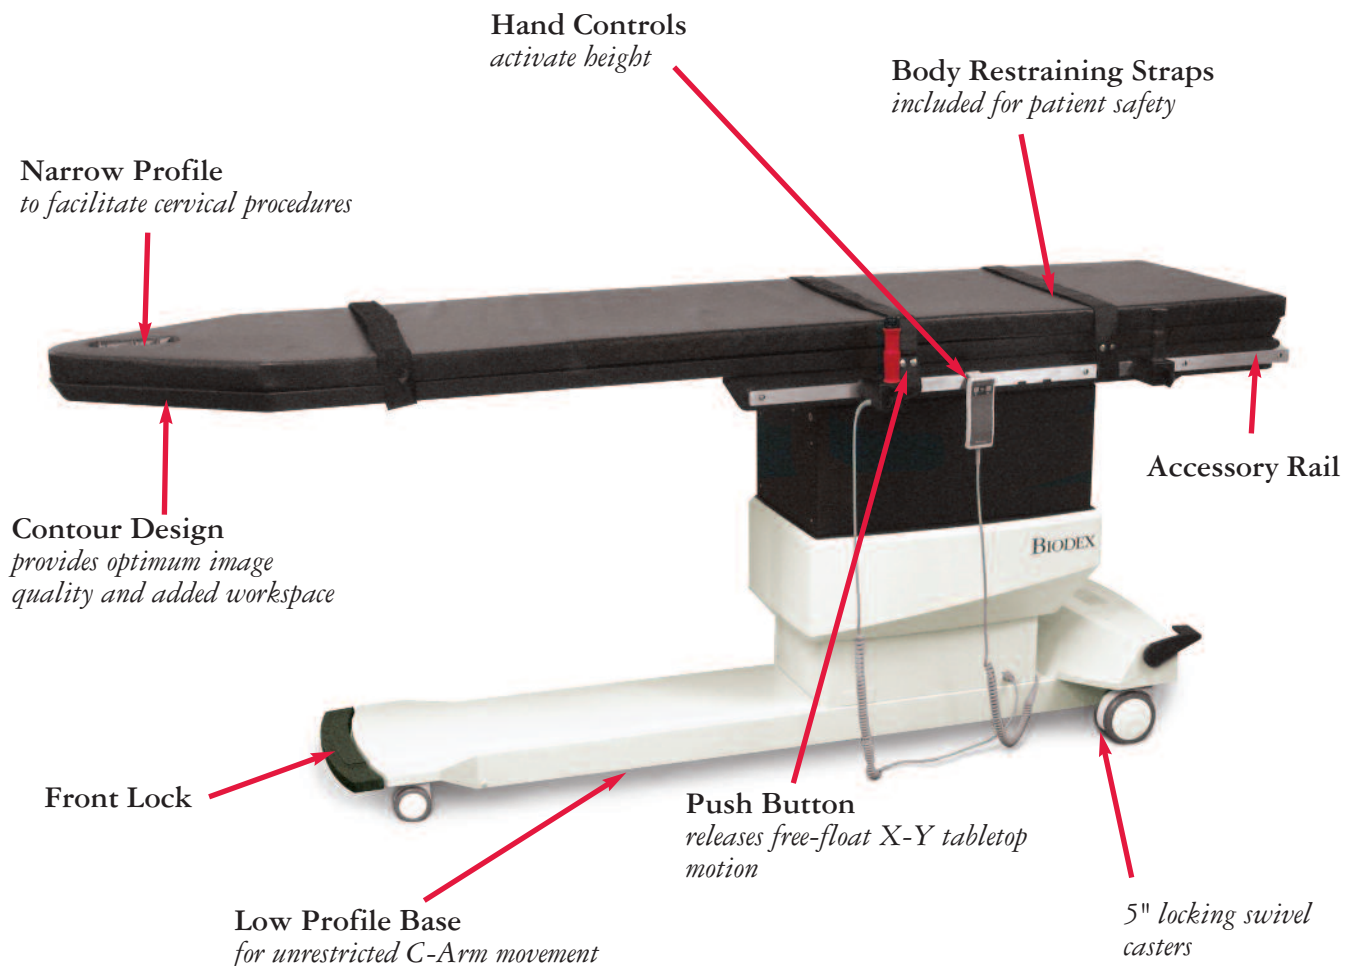

As required by law, all Biodex C-Arm tables are CDRH registered and FDA Device Listed. All motorized tables are ETL product listed to the UL-60601-1 Medical Electrical Equipment Safety Standard.

BIODEX

Biodex Medical Systems, Inc.

20 Ramsay Road, Shirley, New York, 11967-4704, Tel: 800-224-6339 (Int'l 631-924-9000), Fax: 631-924-9338, Email: info@biodex.com, www.biodex.com